



## Rapid test for detection of coronavirus SARS-CoV-2 antigen (Covid 19)


- R&D, designed and made in France
- Accurate and fast detection of specific SARS-CoV-2 antigen in human nasopharyngeal
  - Result within 5-15 minutes
  - Sensitivity : 97,5% ; Specificity : 99,3%
  - Detects the N protein and so forth the new variant of the COVID 19 virus.
- Easy to use
  - No specific equipment required, no training required to undertake this test by the doctors.
- Immunochromatographic test assay designed for the qualitative detection of specific SARS-CoV-2 antigen in human nasopharyngeal swab specimen. It is intended to be used for the detection of SARS-CoV-2 virus infection. The results obtained should not be the sole determinant for clinical decision.
- Certified by the highest Health organisation in France and abroad.

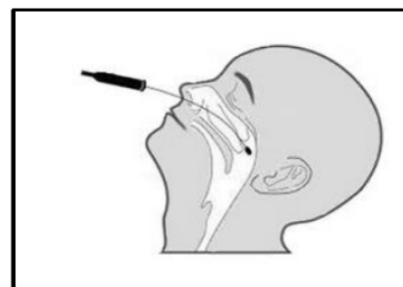

### Assay Process

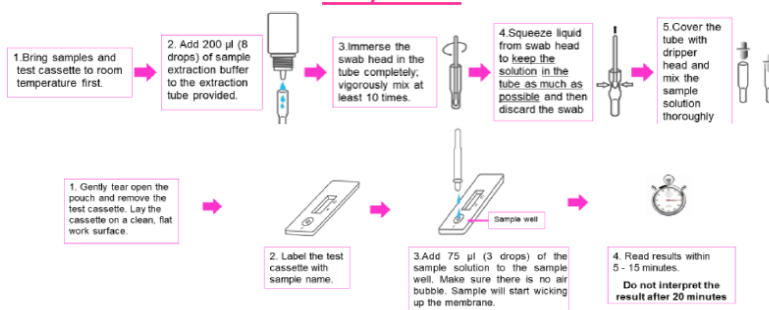

### Interpretation of results

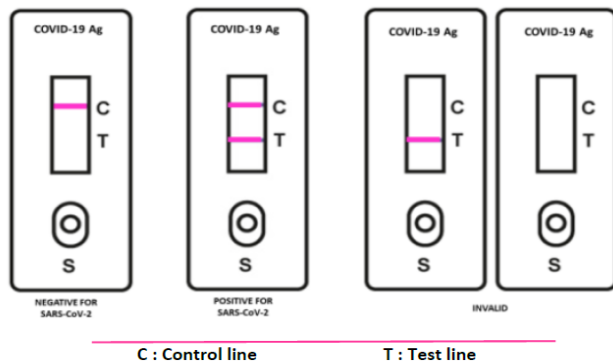

### Antigen Rapid Test (ART)

Reference :  
 COVID19Speed-Antigen Test BSD\_0503-25  
 Packed in 25 units

### Material provided

- 25 swabs
- 25 pcs of COVID-19 Rapid Antigen Test cassette packed in individually aluminum pouch with desiccant
- One bottle of sample Extraction Buffer
- 25 sets of Extraction tube and dropper
- Instruction for use (product insert)

**WARRANTY AND LIMITED LIABILITY :** Failure to follow the assay procedure may derive inaccurate results. In such event, the manufacturer disclaims all warranties expressed, implied or statutory, including the implied warranty of merchantability and the fitness for use. The manufacturer will not be liable for any damage caused by misuse, improper handling and storage, non-compliance with warnings and procedures, damage caused by events occurring after the product is released, failure to ensure the product is in proper condition before use, or any warranty given by independent distributor.